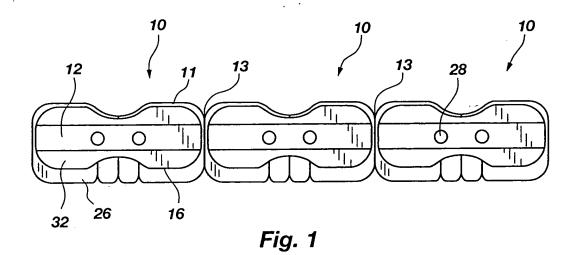
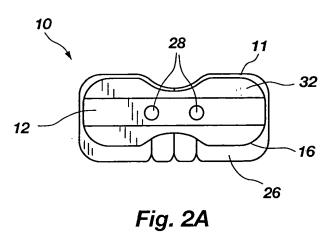
PULSE OXIMETRY SENSOR AND DISPENSING... FUDGE et al.

Appln. No.: Not Yet Assigned Atty. Docket No.: 01-43 C1





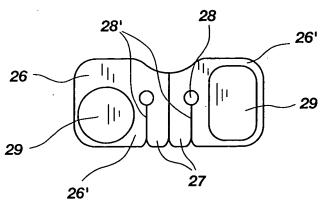


Fig. 2B

PULSE OXIMETRY SENSOR AND DISPENSING... FUDGE et al.
Appln. No.: Not Yet Assigned
Atty. Docket No.: 01-43 C1

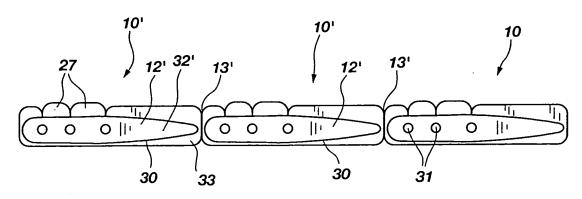
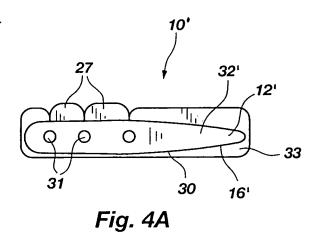


Fig. 3



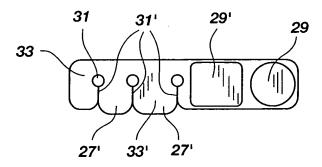
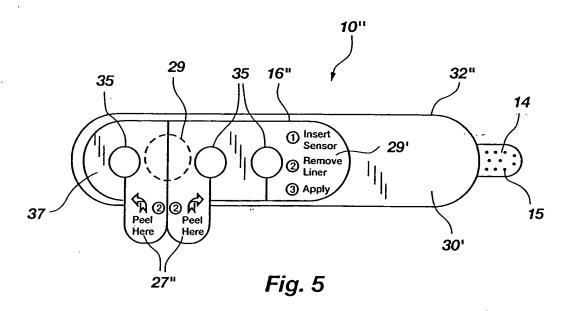
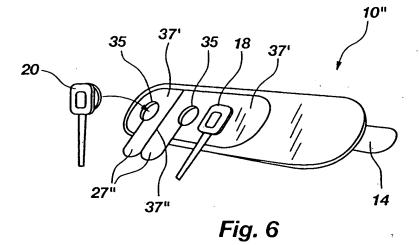


Fig. 4B

Appln. No.: Not Yet Assigned Atty. Docket No.: 01-43 C1

**:** 





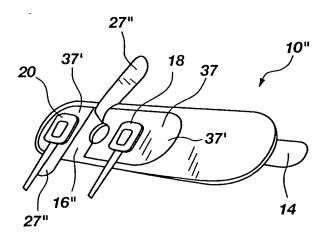


Fig. 7

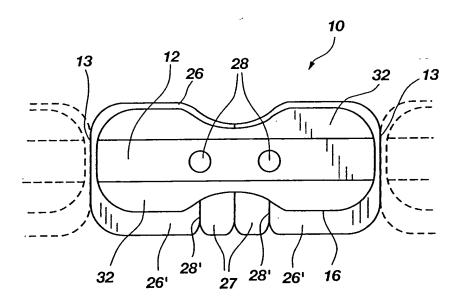
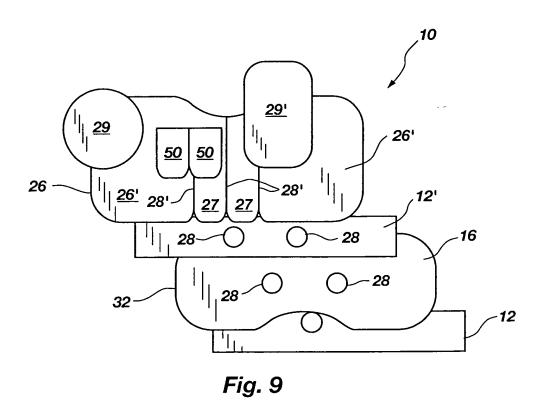


Fig. 8

PULSE OXIMETRY SENSOR AND DISPENSING...
FUDGE et al.
Appln. No.: Not Yet Assigned
Atty. Docket No.: 01-43 C1



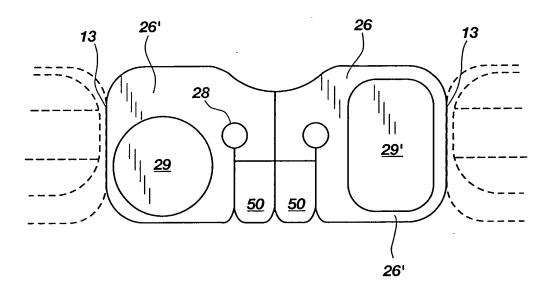


Fig. 10

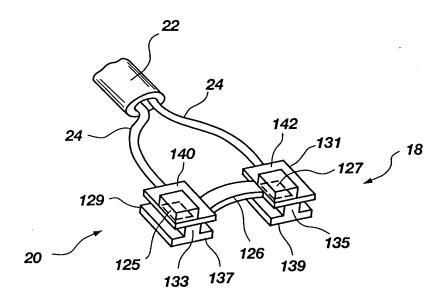


Fig. 11

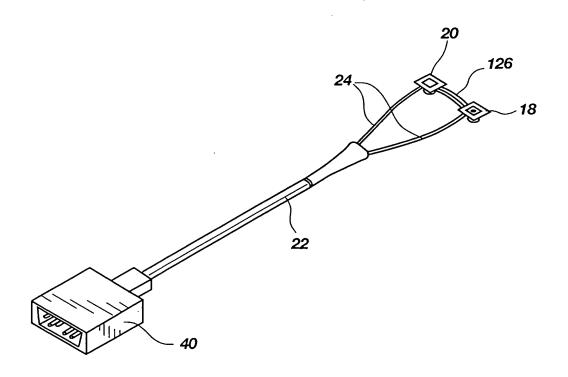


Fig. 12

PULSE OXIMETRY SENSOR AND DISPENSING... FUDGE et al.
Appln. No.: Not Yet Assigned
Atty. Docket No.: 01-43 C1

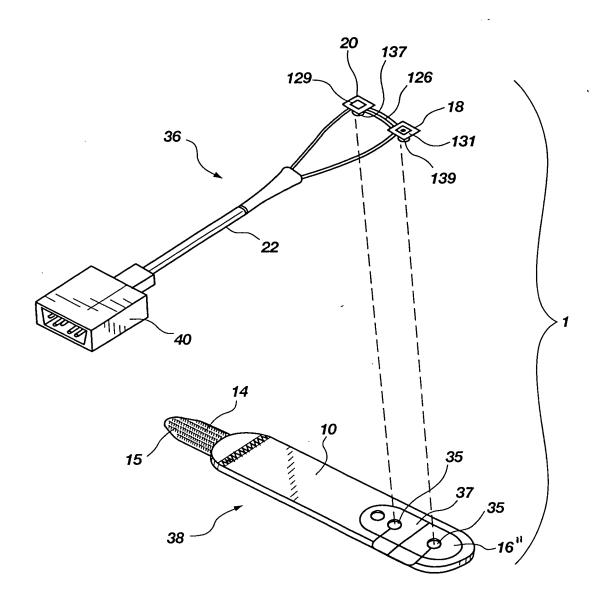


Fig. 13

PULSE OXIMETRY SENSOR AND DISPENSING...
FUDGE et al.
Appln. No.: Not Yet Assigned
Atty. Docket No.: 01-43 C1

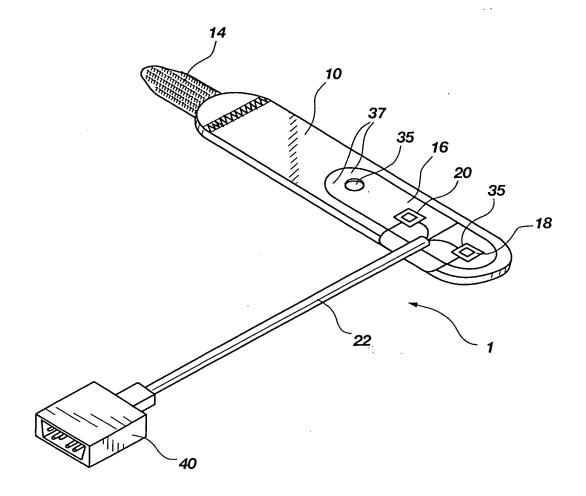


Fig. 14

PULSE OXIMETRY SENSOR AND DISPENSING... FUDGE et al.
Appln. No.: Not Yet Assigned
Atty. Docket No.: 01-43 C1

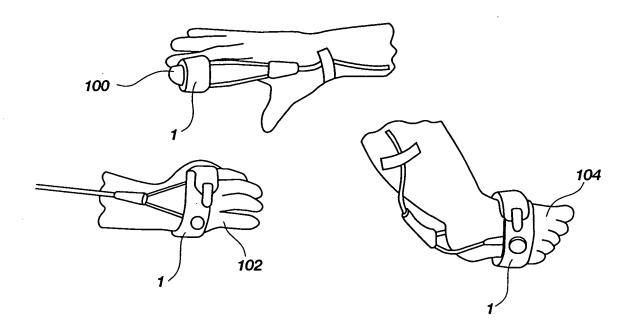


Fig. 15